

| Specifications | |
|--|---|
| Optics | Seya-Namioka mount monochromator, ratio beam |
| Wavelength range | 190 to 1,100 nm |
| Concave diffraction grating | Grooves 600 / mm |
| Spectral bandpass | 5 nm |
| Stray light | 0.07% or less |
| Wavelength accuracy | ±1 nm (484.6 nm) |
| Wavelength setting repeatability | ±0.5 nm |
| Photometric range | Abs: -3.000 to 3.000 Abs |
| | 0 to 300%T |
| Photometric accuracy (certified according to NIST SRM 930) | Conc: 0.000 to 9.999 |
| | ±0.003 Abs (0 to 0.5 Abs) |
| Photometric repeatability (certified according to NIST SRM 930) | ±0.005 Abs (0.5 to 1.0 Abs) |
| | ±0.002 Abs (0 to 1.0 Abs) |
| Wavelength scan speed | 40, 100, 200, 400, 800, 1,200, 2,400 nm / min |
| Baseline stability | 0.0007 Abs/h (260 nm, 2 hours after power-on) |
| Noise level | 0.0002 Abs or less (RMS, 260 nm, 0 Abs) |
| Baseline flatness | ±0.01 Abs (200 to 950 nm) |
| Light source | Xenon(Xe) flash lamp |
| Detector | Silicon photodiode×2 |
| Display | LED with backlight 120 mm×90 mm 320 dot×240 dot |
| Cell holder | 6 cell turret (Automatic) standard, (Single cell holder is optional.) |
| Languages | Japanese, English, Simplified Chinese, and German for stand-alone |
| | Japanese and English for UV Solutions program (PC control) |
| Printer I/F | Centronics interface (Parallel interface) |
| PC I/F | USB 1.1/2.0 (USB connection) |
| Size (main unit) | 355 (W)×425 (D)×235 (H) mm |
| Operating temperature | 15 to 35°C |
| Operating humidity | 25 to 80% (condensation unallowable, within 70% at 30°C or higher) |
| Weight (main unit) | 13 kg |
| Power supply/Power consumption | 100, 115, 220, 230, 240 V 50/60 Hz 60 VA |

| Main software functions | | | |
|------------------------------|---|--------------------------|---------------------------|
| Item | Description | Stand-alone | UV Solutions (PC Control) |
| Photometry | Calibration curve (straight line, linear coefficient) | <input type="checkbox"/> | <input type="checkbox"/> |
| | Calibration curve (quadratic or cubic curve, quadratic or cubic coefficients, line graph) | <input type="checkbox"/> | <input type="checkbox"/> |
| | Automatic measurement using the automated 6-cell turret | <input type="checkbox"/> | <input type="checkbox"/> |
| Wavelength scan | Absorbance, transmittance | <input type="checkbox"/> | <input type="checkbox"/> |
| | Automatic measurement using the automated 6-cell turret | <input type="checkbox"/> | <input type="checkbox"/> |
| | Peak/valley detection | <input type="checkbox"/> | <input type="checkbox"/> |
| | Smoothing | <input type="checkbox"/> | <input type="checkbox"/> |
| | Graph axis switching function | <input type="checkbox"/> | <input type="checkbox"/> |
| | Numerical spectral comparison | <input type="checkbox"/> | <input type="checkbox"/> |
| | Differentiation | <input type="checkbox"/> | <input type="checkbox"/> |
| Time scan | Area calculation function | <input type="checkbox"/> | <input type="checkbox"/> |
| | Absorbance, transmittance | <input type="checkbox"/> | <input type="checkbox"/> |
| | Smoothing | <input type="checkbox"/> | <input type="checkbox"/> |
| Multi-wavelength measurement | Rate calculation function | <input type="checkbox"/> | <input type="checkbox"/> |
| | Absorbance, transmittance | <input type="checkbox"/> | <input type="checkbox"/> |
| Others | Automatic measurement using the automated 6-cell turret | <input type="checkbox"/> | <input type="checkbox"/> |
| | Save function for measurement parameters | <input type="checkbox"/> | <input type="checkbox"/> |
| | Save function for measured data | 50 test | <input type="checkbox"/> |
| | Auto wavelength calibration function | 30 data sets | <input type="checkbox"/> |
| | Automatic start function under a set of specified conditions | <input type="checkbox"/> | <input type="checkbox"/> |

*Microsoft, Windows, Microsoft Excel, and Microsoft Word are the trademarks or registered trademarks of Microsoft Corporation in the USA and other countries.



*This logo is the trademark of Hitachi High-Technologies Corporation throughout the world.

NOTICE: For correct operation, follow the instruction manual when using the instrument.

NOTICE: Although the information contained herein has been reviewed, Hitachi High-Technologies Corporation makes no warranty or representation as to its accuracy or completeness.

Specifications in this catalog are subject to change with or without notice, as Hitachi High-Tech Science Corporation continues to develop new technologies and products for our customers. Not all products are available in all countries. Please contact your local sales representative for details.

Hitachi High-Tech Science Corporation

www.hitachi-hightech.com/global/hhs/

Head Office

24-14, Nishi-Shimbashi 1-chome, Minato-ku, Tokyo 105-0003, Japan



Printed in Japan (H) HSS-E009 2018.3

HITACHI
Inspire the Next



Ratio Beam Spectrophotometer

U-5100

Hitachi High-Tech Science Corporation

ECO-FRIENDLY & CLEAN

For a Beautiful Earth

The concept underlying Hitachi's U-5100 UV-Visible Spectrophotometer is
ECO-FRIENDLY & CLEAN.

The U-5100 delivers a compact, lightweight package with remarkable power savings and
a long life light source.

The U-5100 incorporates every aspect of the technological features of Hitachi's reliability-proven
spectrophotometers while achieving our ultimate goal —

the creation of a new spectrophotometer that is both
ECO-FRIENDLY & CLEAN and provides SUPERIOR PERFORMANCE.



* This display is simulated screen.

ECOLOGY

Long life light source: ▶ P3
Xenon flash lamp Energy saving design ▶ P3

DESIGN

User-friendly interface ▶ P3
A compact, lightweight design ▶ P3

PERFORMANCE


Ratio-beam optical system ▶ P4
Automated 6-cell turret ▶ P4

EASY OPERATION

Automated 6-cell turret equipped as standard ▶ P5
Easy-to-use guidance display ▶ P5
Multi-language display and an export program ▶ P6
PC-based instrument control and data processing ▶ P7


ECOLOGY

Environmental friendly Xe Flash Lamp is a low-power consumption, long-life light source.

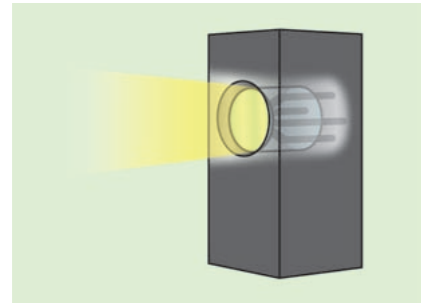


Adoption of a Xenon flash lamp

The adoption of a Xenon flash lamp, a long life lamp*1, eliminates the need for periodic lamp replacement that was necessary in previous models.

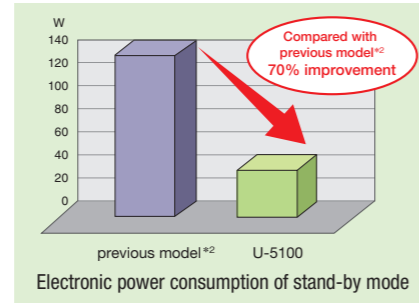

Energy-saving design

Through control of the Xenon flash lamp that emits pulses only during measurement, power consumption is reduced by 70% compared with previous model.

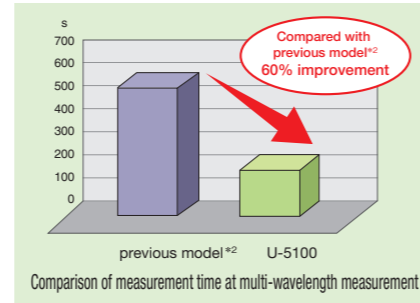

Reduced measurement time

The automatic switching of 6 cells by using an automatic 6-cell turret and a high-speed driving (12,000 nm/min) deliver a substantial reduction in measurement time (approximately 60% reduction). The examples shown in the figure compare*3 the amount of time required to measure 100 samples (5 wavelengths x 20 samples) with a previous model*2, based on biological analysis and quality control on food products.

DESIGN

User-friendly, compact, lightweight design




Pursuit of ease of use

A large, clearly displayed 6-inch LCD is mounted in a simple, arch-shaped form. Cells can be loaded easily from the front of the instrument. The operation panel has a soft keypad that is easy to press, making continuous key operations easy. Letter keys used for character input, such as assigning a file name, are designed to be as easy to use as those on cell phones.



Compact, lightweight design

The U-5100 features a 38% smaller footprint, and the 52% less in weight compared with the previous model*2, which makes it easier to secure an adequate installation space.

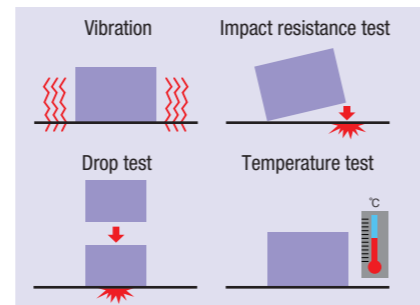

Implementation of strict quality checks

Hitachi's spectrophotometers undergo rigorous quality checks, and the compact, lightweight U-5100 is no exception*4. The U-5100 Maintains the tradition of reliability, for which Hitachi spectrophotometers are well-known.

*1 It is assumed to be ten years under the measurement condition of 1 wavelength, 300 measurements/day, 240 days/year. (Warranty period is one year after installation)
*2 Hitachi Ratio-Beam Spectrophotometer U-1900
*3 Measurement time does not include the amount of time required to load a cell on a holder or a turret.

PERFORMANCE

Compact yet high-performance system with the best baseline stability in its class


The ratio-beam optical system

The ratio-beam optical system incorporated in the U-5100 has a solid track record. This optical system diverts a part of the beam with a half mirror for use by another detector separate from the one used for sample measurements and compensates for changes in energy in the light source. This feature realizes an excellent baseline stability.

In particular, compared with single-beam optical system equipment, the U-5100 provides superior baseline stability during long hours of measurement.


Furthermore, by minimizing the number of mirrors used within, a bright optical system has been created.

In addition, reducing the number of mirrors that deteriorate quickly slows the reduction of beam intensity caused by mirror deterioration.

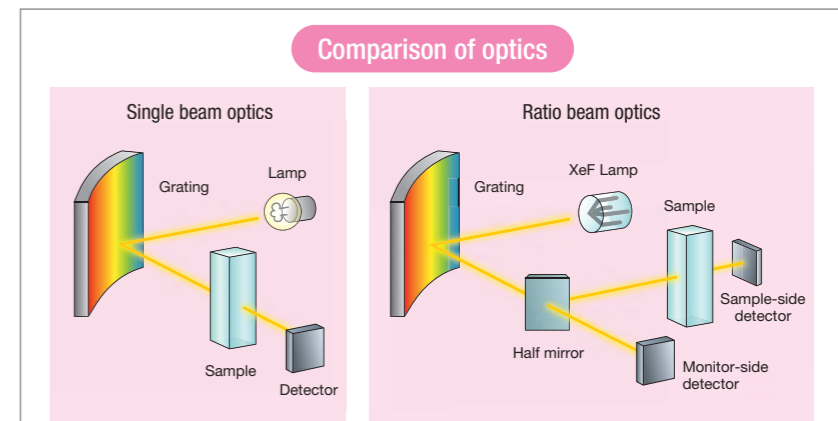

* These diagrams represent design concepts, not actual optical system structures.


Baseline comparison

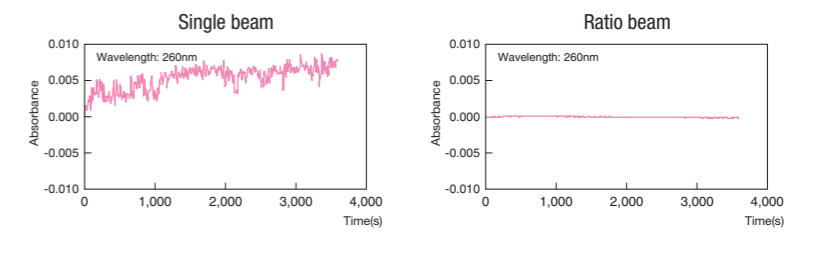

The lowest noise realized by the newly developed light detection circuits: Top of its class.

Incorporating newly developed light detection circuits, the U-5100 offers low-noise performance, the best of its kind in this class of instruments.

When measuring low-concentration samples with a low absorbance, the system demonstrates high stability.

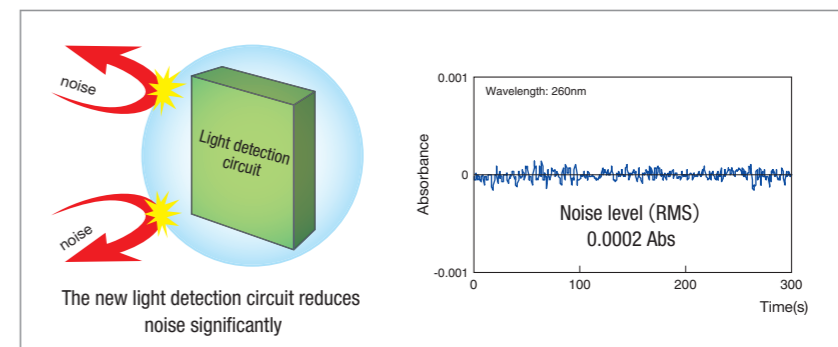

Equipped with an aberration-corrected concave diffraction grating

The U-5100 is equipped with an aberration-corrected concave diffraction grating developed by utilizing Hitachi's unique technology. The U-5100 achieves a high degree of resolution through the removal of astigmatic aberration inherent in the Seya-Namioka monochromator, the most prevalent type of concave diffraction grating.



Concave Diffraction Grating

Performance validation function

This feature allows you to verify the performance of the system easily. Based upon six performance validation parameters, such as "wavelength accuracy," the system provides automatic validation and prints results.

When used in an ISO-certified laboratory, it is important to be able to perform system validations automatically. This makes the U-5100 suitable for use under stringent regulatory requirements.

*4 Hitachi does not guarantee no damage or malfunction when the product is exposed to any of these conditions. Any shock or extreme environmental condition may cause the product to stop functioning properly.


EASY OPERATION

Performing at a Higher Level

The standard automatic 6-cell turret makes performing measurements a breeze.

As part of its standard configuration, the system is equipped with a 6-cell turret which accommodates up to six 10-mm rectangular cells. The system can measure a maximum of six calibration solutions and sample solutions *5, reducing the measurement time and improving the efficiency of your lab.

Stand-alone



6-cell turret

Cell-position guidance display

When using the 6-cell turret for automatic sample measurements, the screen displays sample positions and type of sample to be placed for measurement. For example, when performing a quantitative measurement, the operator can set a calibration or sample solution while checking the "guide on the sample position". Even those users who are new to a spectrophotometer can easily set a cell.



Guidance on a sample loading position

Automatic measurement using a 6-cell turret

Measurement result (calibration curve)

The measurement menu provides the following items, with user-selectable modes:

- Photometry**
- Wavelength Scan**
- Time Scan**
- Data Display**
- Method Menu (up to 50 parameters can be saved)**
- Data Menu (up to 30 data items can be saved)**
- System Setup**
- Performance Check**

Photometry

By measuring a standard solution and creating a calibration curve, users can perform quantitative analyses on unknown samples. Alternatively, quantitative analysis can be accomplished through the input of coefficients. In addition, the system supports multi-wavelength measurement up to six wavelengths to measure absorbance or transmittance, as well as ratio calculations (calculates the purity of DNA by computing the ratio between two wavelengths (A260/A280 and A260/A230)).

Wavelength Scan

Over the 190 to 1100 nm range, the system can measure absorption spectra and transmission spectra. After the measurements, the user can verify the spectral data in great detail by using the peak detection function, the tracing function, the expansion of the abscissa, the ordinate, and the reduced display.

Time Scan

Photometric value (absorbance/transmittance) at a fixed wavelength can be measured in a desired measurement time from 60 to 99900 seconds. This feature can be used to measure the decomposition of the sample from a change in absorbance or the analysis of enzyme reactions.

Data Display

This is a useful mode for the measurement of either absorbance or transmittance at a single wavelength while reading the results. Wavelength and photometric values can be displayed in large characters.

*5 Including samples for setting an auto zero (the operation of adjusting the absorbance to zero)

Standard performance validation and automatic calibration functions assure data reliability.

Automatic self-test at each power on. In addition, the performance validation display allows you to check the results of the automatic validation function, and to check each of six performance validation parameters, assuring a highly reliable system.

Stand-alone

Performance validation

This feature allows you to verify the performance of the system in terms of the following six performance validation parameters:

- Wavelength accuracy
- Baseline flatness
- Wavelength setting repeatability
- Baseline stability
- Noise level
- Hardware (RAM, ROM, lamp, and wavelength scan system)




Screen at power on time



Performance Validation Screen

Standard configuration includes multi-language support

The display language on the model U-5100 can be selected from Japanese, English, Chinese (Simplified), and German. Multi-language support is available for your convenience.

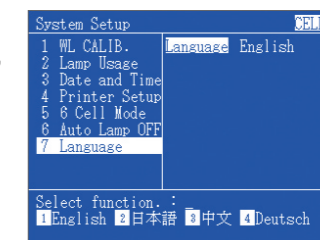

Language Switching Screen

Exporting program

By connecting the model U-5100*6 to a PC containing the export program (P/N 3J2-0290), through the USB interface*7 cable (P/N 3J2-0330), measured data can be output to a printer on the PC or saved in PC files in Microsoft Excel format. Once the desired output parameters are specified, output proceeds by simply pressing the PRINT key on the operation panel of the instrument.

Schematic Diagram

U-5100 --- PC containing the export program --- Printer

A printout through the PC An output file in Excel format

Press the [PRINT] key

Operation panel on the model U-5100

PC Specifications

| | |
|--------------|---|
| Running OS | Windows 7 Professional, (32 bit or 64 bit) Windows 10 Professional (64 bit) |
| CPU | CPU that supports OS |
| Memory | 1 GB or more, 2 GB is recommended (Windows 7) 4GB or more (Windows 10) |
| Hard disk | Free space of 5 GB or more |
| Display | Resolution of 1,920 × 1,080 pixels or higher |
| CD-ROM drive | A drive with a speed of 24x or more is recommended |
| Interface | USB 1.1/2.0 |
| Others | Microsoft Office 2016 |

*6 The firmware (P/N 3J2-5300-05) or later updates are required for the export program. Please contact us for a firmware update for models released earlier than September 2010.

*7 Notice that a single PC can support only a single spectrophotometer, not multiple spectrophotometers.


PC control

PC-based instrument control and data processing


The U-5100 spectrophotometer can be controlled from a PC using the applications program UV Solutions from Hitachi. The U-5100 is connected to the PC through an USB interface^{*8}. In addition to the standalone functions, such as photometry, wavelength scan, and time scan, a variety of data processing and copy / paste / export functions to Microsoft Word and Microsoft Excel are available, supporting your preparation of presentation materials and reports.

Simple operation flow

The measurement operation buttons are arranged on the right side, and a measurement run can be completed in four steps.

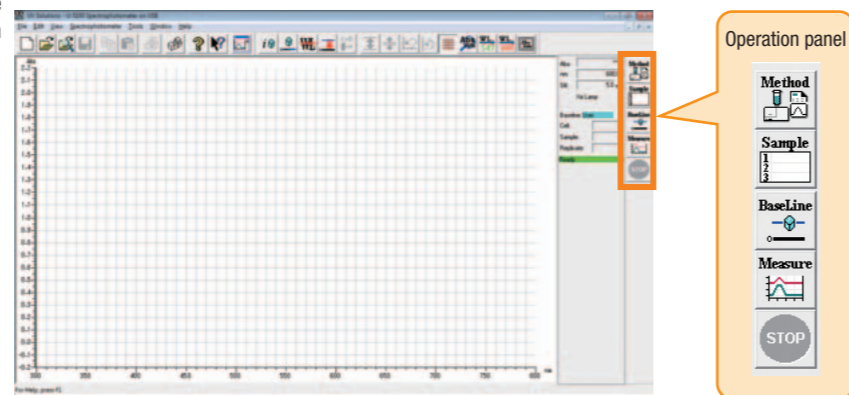

Initial Screen of the UV Solutions Program

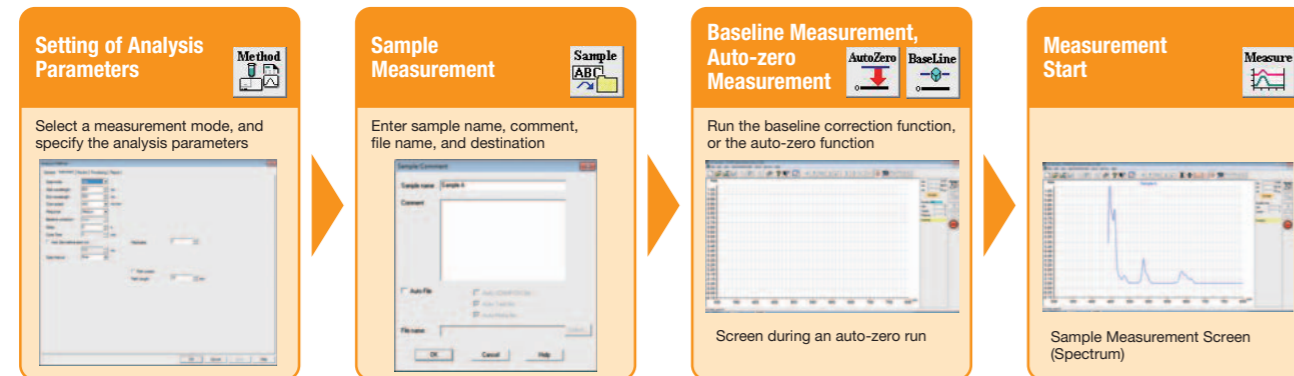


Automatic wavelength scan measurements using the automated 6-cell turret

In addition to the standalone function for automatic measurement, the UV Solutions program allows automatic measurements of up to 6 sample solutions^{*9}, including baseline correction samples, helping to improve work efficiency by reducing the amount of time required for measuring absorption/transmission spectra



Specify measurement parameters, and then load a sample to each cell

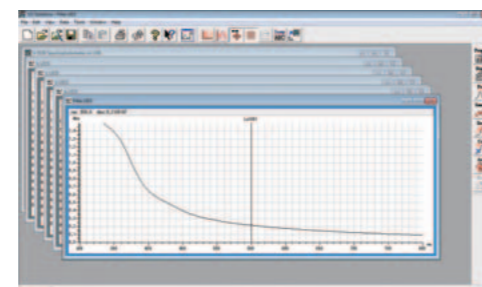

Measurement results

^{*8}The firmware (P/N 3J2-5300-03) or later updates are required for the UV Solutions program. Please contact us for a firmware update for models released earlier than August 2010.
^{*9}Including samples to be used for the auto-zero function (correction needed to adjust the zero level of absorbance).

ACCESSORIES



Auto sipper (P/N 3J2-0105)

The automatic sipper takes a sample from a test tube and can automatically measure it.

| | |
|-----------------------|---------------|
| Minimum sample volume | 0.6 mL |
| Carryover | 1% maximum |
| Cell size | Approx. 50 µL |



Single cell holder (P/N 3J2-0110)

Use this holder to measure with a square cells with a 10-mm optical path. Accommodates one cell.



Rectangular long path cell holder (P/N 3J2-0111)

Use this holder to measure with a square cell with 10, 20, 30, 40, 50, or 100-mm optical paths. Accommodates one cell. The use of cells with long optical paths allows the measurements of low-concentration samples at a high degree of sensitivity.

Micro cell

Micro cells are available for small-sample-volume analysis. Requires a single cell holder (P/N 3J2-0110) and a mask for micro cell (P/N 200-1537).

| Description | P/N | Capacity | Optical path length |
|--------------------------------|----------|---------------|---------------------|
| Micro quartz cell, 10 mm | 124-0357 | 340 to 600 µL | 10 mm |
| Black quartz micro cell, 10 mm | 200-0551 | | |



Ultra-micro volume sample measurement

Ultra-micro volume cells are available for trace analysis. Requires a single cell holder (P/N 3J2-0110) and a Mask for trace sample cell (P/N 3J2-0132).

| Description | P/N | Capacity | Optical path length |
|--------------------------|----------|---------------|---------------------|
| 1.5 µL trace sample cell | 3J2-0120 | 1.5 to 4.0 µL | 1 mm |
| 12 µL trace sample cell | 3J2-0121 | 12 to 40 µL | 5 mm |
| 50 µL trace sample cell | 3J2-0122 | 50 to 90 µL | 10 mm |

Add-on application programs available for the UV Solutions program

Nucleic Acid Measurement program (P/N 3J2-0316)

Helps to verify the extraction and purification of DNA, RNA, and other nucleic acids, which are indispensable for genetic research. Photometric data (at 230, 260, and 280 nm) and calculated results (A_{260}/A_{280} ratio, nucleic acid concentration, protein concentration, and molar concentration) can be displayed collectively, improving the efficiency of purification work.

Report Generator program (P/N 3J2-0312)


Allows customization of data reports. Report items and the size and placement of comments and graphs can be customized. A spreadsheet function is also available for automatic calculations using measured data. Customized reports can be edited and saved as templates. Automatic printout after measurement using a template is also available.

APPLICATION

Quantitation of hexavalent chromium


The figure on the right shows an example of quantitative analysis of hexavalent chromium by diphenylcarbazide absorptiometry. As a result of creating a working curve within 0 to 0.8 µg/mL, a correlation coefficient of 0.9999 was obtained, proving an excellent calibration relationship.

Measuring wavelength: 540 nm
 Concentration of standard solution: 0, 0.04, 0.1, 0.2, 0.5, 0.8 µg/mL

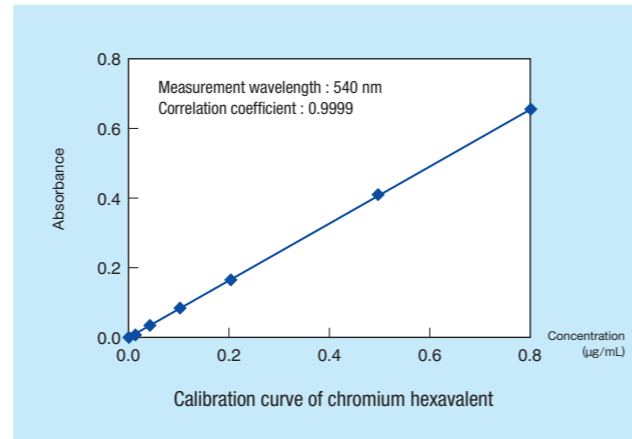

Measurement of total phosphorus

This figure shows an example of quantitative analysis of total phosphorus. As a result of creating a calibration curve within 0 to 2.0 µg/mL, the correlation coefficient of 0.9995 was obtained, proving an excellent calibration curve relationship.

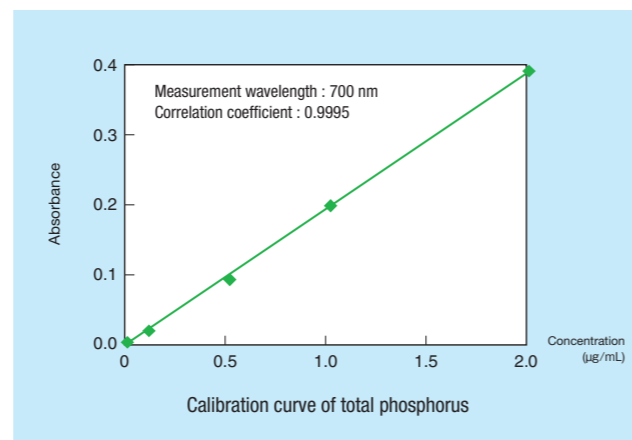


Shortened measurement time using the automated 6-cell turret

The figure on the right shows an example of the quantitative analysis of Food Blue No. 1.

As a result of creating a calibration curve within 0.0 to 2.0 µg/mL, a correlation coefficient of 0.9998 was obtained, proving an excellent calibration relationship.

The time needed for the measurement of 15 unknown samples was 140 s with the model U-5100, which is lower by about 45%, compared with the 260 s needed by a previous model*10

The automated 6-cell turret of model U-5100 allows contiguous measurements of six samples without operator intervention and reduces measurement time.

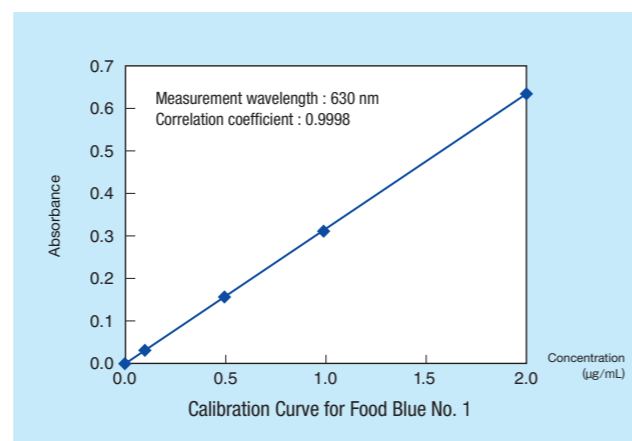

*10 Hitachi Ratio Beam Spectrophotometer U-1900

Advice for Eco Measurement

Our product concept for the model U-5100 is "ECO-FRIENDLY & CLEAN."
 Presented below are issues that you may act on, and advantages that the U-5100 can offer.

Periodic replacement is not needed

The adoption of a Xenon flash lamp contributes to reduced wastes; see page 3 for details.

Waste reduction

Rapid measurement

Automatic measurements contribute to improving the efficiency of your lab; see page 5 for details.

Power savings and CO₂ reduction

Low power consumption

The Xenon lamp emits light only during measurement, contributing to power savings; see page 3 for details.

Power savings and CO₂ reduction

The model U-5100 will help you by performing "eco measurement" for a beautiful Earth